

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problems Mailbox.**

<p>(51) International Patent Classification 6 : A61G 7/05</p>	<p>A1</p>	<p>(11) International Publication Number: WO 99/52487</p> <p>(43) International Publication Date: 21 October 1999 (21.10.99)</p>
<p>(21) International Application Number: PCT/US99/08125</p> <p>(22) International Filing Date: 14 April 1999 (14.04.99)</p> <p>(30) Priority Data: 60/081,698 14 April 1998 (14.04.98) US</p> <p>(71) Applicant: HILL-ROM, INC. [US/US]; 1069 State Route 46 East, Batesville, IN 47006-9167 (US).</p> <p>(71)(72) Applicants and Inventors: MOSTER, Jeffrey, A. [US/US]; 572 Covedale Avenue, Cincinnati, OH 45238 (US). ZERHUSEN, Robert, M. [US/US]; 10186 Owl Creek Road, Cincinnati, OH 45252 (US). HAMILTON, Michael, W. [US/US]; 29252 Chappelow Hill Road, West Harrison, IN 47060 (US). HORNBACH, David, W. [US/US]; 12161 County Line Road, Brookville, IN 47012 (US). CORBIN, Scott, M. [US/US]; 9570 E. North Dearborn Road, Sunman, IN 47041 (US). RIVALLANT, Stéphane [FR/FR]; 9, route des Forges, F-44380 Pornichet (FR).</p> <p>(74) Agent: NIEDNAGEL, Timothy, E.; Barnes & Thornburg, 11 South Meridian Street, Indianapolis, IN 46204 (US).</p>		<p>(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i></p>
<p>(54) Title: COMMUNICATION AND BED FUNCTION CONTROL APPARATUS</p>		
<p>(57) Abstract</p> <p>A communication and control apparatus (30) includes a control unit (46) having a surface (96) accessible to a person on a bed (10), the control unit (46) being coupled to a portion of the bed (10), and a plurality of icons (98) located on the surface (96) of the control unit (46). Each icon (98) represents a separate one of the plurality of controlled functions. The apparatus (30) also includes an indicator associated with each icon (98), a single select switch (84) located on the surface (96) of the control unit (46), and at least one adjustment switch (86, 88) located on the control unit (46) to control the function selected using the select switch (84). The select switch (86, 88) is actuatable to scroll sequentially through the plurality of different functions. The control unit (46) is configured to actuate the indicator corresponding to a function selected as the select switch (84) is actuated to scroll through the plurality of different controlled functions.</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav	TM	Turkmenistan
BF	Burkina Faso	GR	Greece		Republic of Macedonia	TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's	NZ	New Zealand		
CM	Cameroon		Republic of Korea	PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

COMMUNICATION AND BED FUNCTION CONTROL APPARATUSBackground and Summary of the Invention

The present invention relates to a communication and bed function
5 control apparatus for a hospital bed. More particularly, the present invention relates
to a controller mounted to an arm assembly which is coupled to a hospital bed frame
or to a siderail on the bed to improve access to controls by a person located on the
bed.

Several types of controllers are known in the healthcare industry which
10 permit a person located on a hospital bed to activate a number of communication and
control functions, such as adjusting the bed, adjusting the mattress, calling the nurse,
adjusting the room light or reading light, controlling the T.V. or audio functions, or
controlling the telephone. See, for example, U.S. Patent Nos. 5,592,153; 5,239,300;
5,542,138; and 4,680,790. These controllers typically include one or more push-
15 button or pressure sensitive switches, or voice activated controls, to activate various
communication and control functions.

According to one illustrated embodiment of the present invention, a
communication and control apparatus is provided for use by person located on a bed
to control a plurality of different functions. The apparatus includes a control unit
20 having a surface accessible to the person on the bed. The control unit is coupled to a
portion of the bed. The apparatus also includes a plurality of icons located on the
surface of the control unit, an indicator associated with each icon, a single select
switch located on the surface of the control unit, the select switch being actuatable to
scroll sequentially through the plurality of different functions, and at least one
25 adjustment switch located on the control unit to control the function selected using the
select switch. Each icon represents a separate one of the plurality of controlled
functions. The control unit being configured to actuate the indicator corresponding to
a function selected as the select switch is actuated to scroll through the plurality of
different controlled functions. The illustrated indicators corresponding to each icon
30 are lights which are illuminated by the control unit when the function associated with
the icon is selected using the select switch.

Illustratively, the plurality of functions include at least one of calling a
nurse, turning on a light in a room, turning on a reading light, controlling a TV,

controlling a radio, placing and receiving telephone calls, controlling drapes, controlling doors, adjusting a height of the bed, adjusting a configuration of an articulating deck on the bed, adjusting a mattress located on the bed, connecting to the Internet, controlling a video game, controlling a clock, and controlling a electronic
5 notebook. The illustrated control unit also includes at least one of a nurse call switch, a speaker, a reading light, a handle coupled to the control unit to permit the person to move the control unit relative to the bed, a telephone, a card reader, a headphone, and touch screen control panel.

According to another illustrated embodiment of the present invention,
10 a communication and control apparatus is provided for use by a person located on a bed to control at least one function. The bed includes a siderail, and the apparatus includes a control unit configured to control the at least one function, and a linkage including an arm having a first end and a second end, a first coupler configured to the first end of the arm to the siderail about two pivot axes, and a second coupler
15 configured to couple the second end of the arm to the control unit about two pivot axes. The control unit is movable from a storage position adjacent to sidewall to a use position spaced apart from the sidewall by the linkage.

Additional features of the invention will become apparent to those skilled in the art upon consideration of the following detailed description of illustrated
20 embodiments exemplifying the best mode of carrying out the invention as presently perceived.

Brief Description of the Drawings

The detailed description particularly refers to the accompanying
25 drawings in which:

Fig. 1 is a perspective view illustrating a hospital bed with a communication and bed function control apparatus mounted to a frame of the bed adjacent a head end of the bed;

Fig. 2 is an exploded perspective view illustrating an attachment
30 mechanism used to couple an arm assembly of the control apparatus to a corner of the frame of the hospital bed;

Fig. 3 is a sectional view taken along lines 3-3 of Fig. 2;

Fig. 4 is a sectional view taken along lines 4-4 of Fig. 3 illustrating further details of the attachment mechanism;

Fig. 5 is a bottom view of Fig. 4;

Fig. 6 is a front view of one embodiment of a control unit of the present invention;

Fig. 7 is a side elevational view of the control unit of Fig. 6;

Figs. 8-11 illustrate other embodiments of control units in accordance with the present invention;

Fig. 12 illustrates the control unit of Fig. 11 mounted to a siderail of a bed with a pivoting and telescoping arm mounting assembly;

Figs. 13A-19 illustrate additional embodiments of control units of the present invention;

Figs. 20 and 21 are perspective views of another control unit which includes a plurality of communication and bed function control buttons on one side of the control unit as shown in Fig. 20 and a telephone on the other side of the control unit as shown in Fig. 21;

Fig. 22 illustrates the control unit of Figs. 20 and 21 coupled to a siderail of a bed;

Fig. 23 illustrates another embodiment of a control unit in accordance with the present invention;

Fig. 24 illustrates the control unit of Fig. 23 pivotably mounted to a siderail of the bed;

Figs. 25-27 illustrate further embodiments of control units of the present invention;

Fig. 28 illustrates yet another control unit mounted on a bed siderail;

Fig. 29 illustrates pivotable movement of the control unit of Fig. 28 relative to the siderail;

Fig. 30 illustrates the control unit fully pivoted away from the siderail by a pivot arm apparatus;

Figs. 31-35 illustrate another embodiment of a siderail mounted control unit; and

Fig. 36 is a block diagram of a connection to a nurse call system.

Detailed Description of the Drawings

Referring now to the drawings, Fig. 1 illustrates a hospital bed 10 having a base frame 12 and casters 14 coupled to the base frame 12. An articulating support deck 16 is coupled to the base frame 12 in a conventional manner. It is understood that the control units of the present invention may be used with any type of bed configuration. The illustrated bed 10 includes a head end 18 and a foot end 20. A mattress 22 is located on the support deck 16 for supporting a person on the bed 10. Siderails 24 are located on opposite sides of the mattress 22 in a conventional manner.

Fig. 1 illustrates a communication and bed function control apparatus 30 mounted to an outer frame member 32 of the bed 10 by an attachment mechanism 34 as best illustrated in Figs. 2-5. The communication and bed function control apparatus 30 further includes a first arm 36 connected to a pivot cylinder 38. A second arm 40 is coupled to first arm 36 by a pivot joint 42. A flexible tube 42 is coupled to second arm 40. A curved attachment portion 44 is coupled between the flexible portion 42 and a control unit 46.

The attachment mechanism 34 shown in Figs. 2-5 includes an inner mounting plate 48 having upturned tabs 50 which are formed to include apertures 52. Attachment mechanism 34 further includes an outer mounting plate 54 having a curved portion 56 formed to include mounting apertures 58. Outer mounting plate 54 further includes an extended support portion 60 having an aperture configured to receive the cylindrical member 38 so that cylindrical member 38 can pivot about a longitudinal axis 62 as shown by double-headed arrow 64 in Fig. 2. A bottom surface of inner mounting plate 48 includes a clamp 72 which is also configured to receive the cylindrical member 38 as shown in Fig. 5. An adjustment screw 74 is configured to adjust the tightness of clamp 72 on the cylindrical member 38. Clamp 72 is spaced apart from support portion 60 of the outer mounting plate 54 to hold the cylindrical member 38 for rotation about the longitudinal axis 62 as discussed above.

Fasteners such as bolts 66 are configured to extend through apertures 58 formed in outer mounting plate 54, through apertures 68 formed in frame member 32 of the bed 10, and through apertures 52 of inner mounting bracket 48 to secure the attachment mechanism 34 to the bed 10. Illustratively, nuts 70 hold the bolts 68 in place. It is understood that other types of fasteners including rivets, screws, clamps, etc. may be used to secure the attachment mechanism 34 to the bed 10.

The control unit 46 is further illustrated in Figs. 6 and 7. The control unit 46 includes a body portion 80 having control buttons 82 including a "select" button 84, a "-" or down button 86, and a "+" or up button 88. Control unit 46 further includes a large aperture 90 configured to define a grip handle 92. A light 94 is
5 located within the handle 92 to provide light for reading or other activities for the person on the bed 10. A modular control panel 96 includes indicators or icons 98 for the various control functions performed by the control unit 46. In addition, volume or level indicators 100 are also provided on the panel 96. Each of the icons and indicators 98 and 100 may be separately illuminated to provide an indication of which
10 function is being controlled as discussed below.

The bed articulation control indicator 102 is also located on the panel 96. Separately illuminatable movement levels are shown at 104, 106, and 108. A nurse call button 110 extends across a top edge of the control unit 46. Nurse call button 110 may be illuminated or made from a different color material, if desired, to
15 make the nurse call button 10 stand out from the remainder of the control unit 46. Illustratively, the nurse call button 110 is illuminated when it is activated. The location of the nurse call button 110 which extends substantially along an entire top edge of the control unit facilitates activation of the nurse call switch 110.

A microphone 112 is located on control panel 96 for phone use or for
20 communicating with a remote nurse station. At least one speaker 114 illustratively is located within the control unit 46. Speakers 114 and microphone 112 permit hands-free use of the telephone or communications with the nurse station. The speakers 114 also provide radio and T.V. audio. A mounting bracket 113 is located on a rear surface 115 of control unit 46.

25 When the select button 84 is pressed, the controller scrolls through the various icons 98 on the control panel to provide a visual indication of which function is currently being controlled by the control unit 46. Once the particular icon 98 is illuminated, adjustments can be made using the up and down buttons 88 and 86.

Each time a select button 84 is pressed, the controller scrolls to the
30 next function and highlights or illuminates the icon 98 corresponding to the function that is currently being controlled. An LED or other light source is used to provide illumination of the particular icon to provide the indication of the function being controlled. Once the radio icon, television icon, light control icon or other icon is

illuminated, the up and down buttons 88 and 86 are pressed to adjust the volume, intensity of the light, etc. Individual level indicators 100 are then separately illuminated to provide an indication of the volume level or intensity level of the light, etc. When the bed functions 102 are selected, an operator presses the "+" up button 88 to raise the identified section of the bed 10. The "-" down button 86 is pressed to lower the identified section of the bed. Illustratively, buttons 84, 86 and 88 are momentary contact switches. Therefore, as long as the buttons 86 and 88 are held down, the bed function will continue to operate. When the buttons 86 and 88 are released, the bed function ceases to operate.

Another embodiment of a control unit 120 is illustrated in Fig. 8. The control unit 120 is illustratively mounted on an arm 122 coupled to the bed 10 in any manner. It is understood that any attachment mechanism or number of arms may be used to mount the control unit 120 to the bed 10. Control unit 120 includes a body portion 124 formed to include an aperture 126 defining a grip handle 128 along a side of the control unit 120. A nurse call switch 130 is mounted to a top portion of handle 128. A nurse call switch 130 may be actuated by a thumb of the operator while the operator is gripping the handle 128. Nurse call switch 130 is illustratively illuminated when pressed. Control unit 120 includes individual buttons 132 for selecting the T.V., radio, lights, etc for control. Separate up and down buttons 134 and 136 are provided to control the selected function. Articulation control buttons 138 are separate from the other function buttons 132. The control unit 120 further includes a speaker 140 for hands-free telephone and nurse communication. A light 142 is located within the body portion 124 of control unit 120 adjacent a bottom surface.

Fig. 9 illustrates yet another embodiment of a control unit 144. The control unit 144 includes a curved support arm 146 coupled to another arm 148 by a pivot connection 150. A nurse call button 152, function control switches 154 for the radio, T.V., bed operation, and lighting, and up and down control buttons 156 and 158 are located along a top surface of the arm 146. When a particular function switch 154 is selected, that selected function is controlled using up and down switches 156 and 158. A reading light 160 is located within a body portion 162 of the control unit 144 which extends downwardly from the arm 146. Body portion 162 further includes bed articulation controls 164. One or more speakers 166 are located within the body portion 162.

Fig. 10 illustrates still another control unit 168 of the present invention. The control unit 168 includes a curved support arm 170. A distal end 172 of arm 170 provides a grip handle for movement of the control unit 168. Function selection switches 174 for T.V., radio, lights, etc. are located on a front surface of the arm 170 facing the operator. Up and down control switches 176 and 178 are also located on the front surface of the control arm 170 for easy access. A nurse call switch 180 is located on a corner portion of the arm 170. A speaker 182 for hands-free telephone use is located below the nurse call switch 180 within the arm 170. A body portion 184 is coupled to the arm 170. Body portion 184 includes bed articulation controls 186 and a light 188.

Still another control unit 190 is illustrated in Figs. 11 and 12. Control unit 190 is illustratively movable from a first position illustrated by dotted lines 190 in Fig. 12 in which the control unit 190 provides a central portion of a siderail 192. In other words, the control unit 190 fits within a gap formed between spaced-apart portions of the siderail 192 when the control unit is in a first storage position. The control unit 190 is coupled to a portion of the siderail 192 by a mounting arm 194 and a pivot connection 196 which is coupled to siderail 192. Pivot connection 196 and arm 194 are movable to the position shown in Fig. 12 so that the control unit 190 moves away from the siderail 192. The arm 194 is a telescoping arm to permit adjustment of the location of the control unit 190. Control unit 190 is rotatably coupled to an end of the arm 194. Arm 194 can also pivot away from the bed 10 so that the control unit 190 may be used from outside the bed, such as when an operator is located in a chair next to the bed. The control unit 190 is typically stored in the siderail 192 and is moved outwardly only when desired.

A telephone handset 198 is positioned along top surface 200 of the control unit 90. Control unit 190 includes a body portion 201. Separate function selection switches 202 are provided for the T.V., radio, lights, etc. Up and down control switches 204 and 206 are located adjacent the function selection switches 202. Bed articulation control switches 208 are also located on the body portion 201. A card reader slot 212 is provided on the body portion 201. The card reader 212 is used to read a phone card, credit card, or debit card for using the T.V. or telephone. In addition, the reader 212 may be a smart card reader for reading information available

on a conventional smart card. A nurse call button 212 extends along the entire front of body portion 201.

Another embodiment of a control unit 214 is illustrated in Figs. 13A and 13B. As best illustrated in Fig. 13A, control unit 214 includes a body portion 216
5 having a generally cylindrical mounting tube portion 218 configured to mount the control unit 214 to a top rail on a siderail or other device for rotation about a longitudinal axis 220. Body portion 216 includes a nurse call switch 222 and separate function control switches 224 for T.V., radio, lighting, etc. Separate up and down control switches 226 and 228 are provided to adjust the functions once a particular
10 function is selected using switches 222 as discussed above. Separate bed articulation control buttons 230 are formed on an upper portion of body 216. A phone 230 is located along mounting tube 218. A card reader slot 232 is provided above phone 230.

Fig. 13B illustrates the control unit 214 mounted to a top bar 234 of a
15 siderail. Control buttons (not shown) are also located on surface 236 of control unit 214. Therefore, functions such as bed articulation functions may be used when the control unit 214 is pivoted downwardly to a storage position adjacent the siderail.

Another embodiment of a control unit 238 is illustrated in Fig. 14. Control unit 238 includes a body portion 240. Body portion 240 includes first and second apertures 242 and 244 configured to define first and second grip handles 246
20 and 248 to permit gripping of the control unit 238 from either side. A nurse call switch 250 is located along a top surface of the control unit 238 between the first and second grips 246 and 248. A reading light 252 is located on the control unit 238 between the first and second grips 246 and 248 as shown. Speakers 254 are located
25 adjacent each of the grips 246 and 248. Control unit 238 further includes function selection switches 256, up and down control buttons 258 and 260, and bed articulation control buttons 262.

Figs. 15 and 16 illustrate a further control unit 264. Control unit 264 includes a body portion 266 coupled to a control arm 268. Illustratively, arm 268 may
30 be mounted to the headboard of the bed via a mechanical clip attachment. A telephone 270 is mounted to a first side of control unit 264. A speaker 272 and a microphone are also provided for hands-free telephone use. Separate function selection switches 274 and up and down control switches 276 and 278 are located on

the body portion 266 of control unit 264. Bed articulation control switches 280 are also located on the body portion 266. A nurse call switch 282 is located on a top surface of control unit 264. A headphone 284 is stored within a receptacle 286 on a second side of the control unit 264 opposite from the phone 270. Illustratively, a retractable cord 286 connects the headphone 284 to the control unit 264. The removable headphone 284 may be used with the audio system for watching T.V. or listening to the radio. In addition, the headphone 284 may be used for hands-free telephone or for communication with the nurse station. A phone card reader slot is located beneath the phone 270.

Another control unit 290 is illustrated in Fig. 17. Control unit 290 is mounted on arm assembly 292 having a telescoping and rotatable L-shaped member 294. L-shaped member 294 is rotatable about an axis 293 and movable back and forth in the direction of double-headed arrow 295 to adjust the length of the arm 292. Control unit 290 is mounted to an arm of the L-shaped member 294 and is rotatable about axis 296. Control unit 290 includes a body portion 298 having separate bed function selection switches 300. Up and down control buttons 302 and 304 are located adjacent the bed function selection switches 300. Bed articulation control switches 306 are also located on the control unit 290. Body portion 298 of control unit 290 is cantilevered from the arm of L-shaped member 294 so that the body portion 298 overhangs the horizontal support arm 292. A nurse call button 308 extends along a top surface of the control unit 290. A reading light 310 is located on a downwardly inclined surface 312 formed on the body portion 298. A speaker 314 is also located within the body portion.

A further control unit 316 is illustrated in Fig. 18. Control unit 316 includes a body portion 318 mounted to an arm 320. Control unit 316 includes a first nurse call button 322 extending along a top edge and top corner of the body portion 318. A second nurse call button 324 extends along a side edge and bottom corner of the body portion 318. Separate function control selection switches 326 are provided for selecting functions to be controlled as discussed above. Up and down control switches 328 and 330 are located adjacent the function selection switches 326. Control unit 316 includes a handle 332 and a reading light 334 located along a bottom surface of body portion 318. Separate bed articulation control buttons 336 are

provided. Control unit 316 further includes a speaker 337 located within the body portion 318.

An additional control unit 338 is illustrated in Fig. 19. Control unit 338 includes a body portion 340. Body portion 340 is mounted to an arm 342. A nurse call switch 344 extends along a top surface and upper corner of the body portion 340 of the control unit 338. Separate function selection switches 346 are provided on the body portion 340 to select between various functions to be controlled. A handle 348 is coupled to the body portion 340. The handle is rotatable about its longitudinal axis as illustrated by double-headed arrow 350. Rotation of the handle 340 adjusts various selected functions similar to the up and down buttons discussed above. For instance, if a user wants to listen to the radio, the radio selection switch 346 is pressed. Once the radio function is chosen, the operator turns the handle to the left or the right to change stations. Once the station is selected, the radio switch 346 is again pressed. The handle 348 is then used to adjust the volume from a speaker 352 by turning the handle to the left or the right. The handle 348 illustratively rotates less than 360° and activates the up switch or the down switch in an arc based on appropriate ergonomics. The handle 348 is illustratively biased to the center position. Bed articulation control switches 354 are also located on the body portion 340. In addition, a reading light 356 is located on the control unit 338.

Another embodiment of the present invention is illustrated in Figs. 20-22. A control unit 358 includes a body portion 360 having a nurse call switch 362, function selection switches 364, and up and down control switches 366 and 368. A cord 370 is connected to the control unit 358. A bottom side of the control unit 358 is illustrated in Fig. 21. The bottom side of the standard telephone handset including a microphone 372, a speaker 374, and a touch tone control pad 376. Bed articulation controls can also be located on the control unit 358, if desired. Control unit 358 is designed to be stored on a siderail 380 of a bed 10 as illustrated in Fig. 22. When in the storage position, the user can operate the control function switches. The control unit 358 is removed to use the telephone. Therefore, the control unit 358 is integrated with the bed 10 and bed function controls are located on the back side of the phone. A phone card slot is also located on the control unit 358. A retention mechanism on the siderail 380 is illustratively configured to hold the control unit 358 within the siderail 380. The control unit 358 may be held in place by a friction fit connector or

by pins or levers which hold the control unit 358 in place and which are released by buttons or handles to remove the control unit 358.

Another control unit 382 is illustrated in Figs. 23 and 24. Control unit 382 includes a body portion 384 mounted to an arm 386. Illustratively, the arm 386 is pivotably coupled to a siderail 390 as shown in Fig. 24. The arm is movable from an upright position shown in Fig. 24 to a downwardly pivoted storage position in which the control unit 382 is nested within the siderail 390.

The control unit 382 includes separate function selection switches 392. Up and down control switches 394 and 396 are also located on the body portion 384. Speakers 398 are also located on the body portion 384. A nurse call switch 400 is located along a side of the control unit 382. Separate bed articulation control switches 402 are also provided. A microphone 404 is included for hands-free telephone and nurse communications.

Yet another control unit 406 is illustrated in Fig. 25. Control unit 406 includes a body portion 408 mounted to a support arm 410. Separate function selection switches 412 are located on the body portion 408. A handle 414 is rotatable about axis 416 to provide high/low or up/down control for each function selected similar to the handle 348 discussed above with reference to Fig. 19. The handle 414 is coupled to an L-shaped connector member 418 extending downwardly from body portion 408. A light 420 is formed on a corner of the L-shaped member 418. A nurse call switch 422 is located on a side edge of the body portion 408. Nurse call 422 may also be located along a top surface of body portion 408, if desired. A speaker 424 and separate bed articulation controls 426 are also located on the body portion 408 of control unit 406. The handle 414 is located in a generally horizontal orientation when in use. The handle 414 permits the operator to move the control unit 406 as well as to adjust the control functions in a manner similar to up and down switches discussed above.

Another illustrated control unit 430 is illustrated in Fig. 26. Control unit 430 includes a body portion 432 mounted to a control arm 434. Body portion 432 includes a central aperture 436 and a rotatable grip portion 438. Grip portion 438 is used to adjust the high/low or up/down controls. Separate function selection switches 440 are located on the body portion 432. A nurse call switch 442 is located along a top surface of the body portion 432. Speakers 444 are located on opposite

sides of the body portion 432. In this embodiment, the rotatable control grip 438 is located in a center portion of the control unit 432. A light 446 is also coupled to the body portion 432.

Yet another embodiment of the control unit 450 is illustrated in Fig.

- 5 27. Control unit 450 includes a body portion 452 mounted to an arm 454. Control unit 450 includes separate function control switches 456 and two pairs of up and down controls 458 and 460 on opposite sides of the control unit 450. Speakers 462 are located near a top portion of control unit 450. A nurse call switch 464 is located along a top surface of control unit 450. A light 466 is located along a bottom portion of
10 control unit 450.

A touch screen control panel 468 is located in a center portion of control unit 450. A control screen 460 provides flexibility for controlling various types of menu driven functions. Different programs may be installed for operation of different functions. The screen 468 is also used for connection to an Internet site to
15 play video game products. A computer mouse control apparatus or keyboard may be connected to the control unit, if desired. In addition, the control buttons on the control unit 450 may be used to control connection to the Internet or the video games. Control screen 468 may be a television screen, computer screen, or touch screen control panel.

- 20 Figs. 28-30 illustrate a siderail mounted control unit 470. The control unit 470 is configured to be integrated with the siderail 472. In a nested storage position shown in Fig. 28, the control unit 470 is located adjacent the siderail. Control buttons 474 to control functions of the bed or room, bed articulation, nurse call, telephone, etc. are integrated into the control unit 470 in the manner discussed
25 above. The control buttons 474 are located on a generally planar surface of the control unit 470 the is aligned at a transverse angle relative to a plane of the siderail 472. Therefore the control buttons 474 are aligned at an angle toward the head of the person on the bed 10.

- An operator can grip the control unit 470 and pivot control unit 470
30 outwardly from the siderail 472 as illustrated in Fig. 29. As shown in Fig. 30, a support arm 476 is pivotably coupled to the siderail 472. A first pivot connection is configured to connect the arm 476 to the siderail 472 about pivot axis 480. A sleeve 482 is rotatably coupled to mounting portion 478. Arm 476 is pivotably coupled to

sleeve 482 about axis 484. Therefore, arm 476 can move up and down and forward and backward relative to the siderail 476 as shown in Fig. 30. An opposite end of arm 476 is pivotably coupled to the control unit 470. Control unit 470 includes additional controls 486 on an opposite side of the control unit 470 from controls 474 for use
5 when the control unit 470 is in its outwardly extended position. The illustrated siderail 472 includes a cylindrically shaped top rail 473, a center rail 475 and a bottom rail 477. The control unit 470 includes a curved top surface 479 configured to receive the curved profile surface of the top rail 471. The control unit 470 also includes first and second recessed portions 481 and 483. The first recessed portion 481 is
10 configured to receive the arm 476 when the control unit 470 is moved to the storage position of Fig. 28. The second recessed portion 483 is configured to receive the center rail when the control unit 470 is moved to the storage position of Fig. 28.

Another embodiment of the present invention similar to Figs. 28-30 is illustrated in Figs. 31-35. A different type of pivot linkage 493 is used to connect a
15 control unit 490 to a siderail 492. A support channel 494 of linkage 493 is pivotably coupled to the siderail 492 about axis 496. First and second arms 498 and 500 are pivotably coupled to support channel 494 by pivot connections 502 and 504, respectively. Arms 498 and 500 can move up and down about pivot axes 502 and 504, respectively, as illustrated in Fig. 33 to raise and lower the control unit 490
20 relative to the siderail 492. Arms 498 and 500 are also pivotably coupled to flanges 506 on the control unit 490 by connector 509. Therefore, control unit 490 can rotate about axis 508 relative to arms 498 and 500. Arms 498 and 500 also pivot about pivot connections 511 and 513 coupled to connector 509. Linkage 493 therefor permits the control unit 490 to move forward and backward and up and down relative to the
25 siderail 492. Illustratively, control unit 490 includes function control buttons 510 and bed articulation control buttons 512. A speaker 514 is coupled to the siderail 492. A light 516 is located adjacent the speaker 514. The control unit 490 includes a curved top surface 491 configured to receive the curved profile surface of the top rail of siderail 492.

30 Fig. 36 is a block diagram illustrating connection of the various control units to a nurse call interface on the wall of the hospital room. The control units may be either on the left hand or right hand siderail as illustrated at blocks 520 and 522. The control units are coupled to a communication junction box 524 on the hospital

bed 10. Junction box 524 is coupled to a microcontroller interface 526 which is coupled to a nurse call interface located on the hospital wall as illustrated at block 528. Therefore, the control units of the present invention can communication with the nurse call system and/or with the electrical communication network of the hospital to
5 transmit and receive information from remote locations.

Although the invention has been described in detail with reference to a certain illustrated embodiment, variations and modifications exist within the scope and spirit of the invention as described and as defined in the following claims.

CLAIMS:

1. A communication and control apparatus for use by person located on a bed to control a plurality of different functions, the apparatus comprising:
 - a control unit having a surface accessible to the person on the bed, the
 - 5 control unit being coupled to a portion of the bed;
 - a plurality of icons located on the surface of the control unit, each icon representing a separate one of the plurality of controlled functions;
 - an indicator associated with each icon;
 - a single select switch located on the surface of the control unit, the
 - 10 select switch being actuatable to scroll sequentially through the plurality of different functions, the control unit being configured to actuate the indicator corresponding to a function selected as the select switch is actuated to scroll through the plurality of different controlled functions; and
 - at least one adjustment switch located on the control unit to control the
 - 15 function selected using the select switch.
2. The apparatus of claim 1, further comprising an arm assembly having a first end coupled to the control unit and a second end coupled to the bed.
3. The apparatus of claim 2, further comprising an attachment mechanism coupled to the arm assembly, the attachment mechanism being configured
- 20 to secure the arm assembly to a frame member of the bed.
4. The apparatus of claim 1, wherein the plurality of functions include at least one of calling a nurse, turning on a light in a room, turning on a reading light, controlling a TV, controlling a radio, placing and receiving telephone calls, controlling drapes, controlling doors, adjusting a height of the bed, adjusting a
- 25 configuration of an articulating deck on the bed, adjusting a mattress located on the bed, connecting to the Internet, and controlling a video game.
5. The apparatus of claim 1, further comprising a nurse call switch coupled to the control unit.
6. The apparatus of claim 5, wherein the control unit includes a
- 30 top surface, a bottom surface, and first and second side surfaces extending between the top and bottom surfaces, the nurse call switch being located on the top surface of the control unit.

7. The apparatus of claim 6, wherein a portion of the nurse call is also located on one of the first and second side surfaces of the control unit.

8. The apparatus of claim 5, wherein the control unit includes a top surface, a bottom surface, and first and second side surfaces extending between the top and bottom surfaces, the nurse call along one of the first and second side surfaces of the control unit.

9. The apparatus of claim 1, further comprising a speaker coupled to the control unit.

10. The apparatus of claim 1, further comprising a reading light coupled to the control unit.

11. The apparatus of claim 1, wherein the indicator corresponding to each icon is a light which is illuminated by the control unit when the function associated with the icon is selected using the select switch.

12. The apparatus of claim 1, further comprising a level indicator light located on the surface of the control unit.

13. The apparatus of claim 1, further comprising a handle coupled to the control unit to permit the person to move the control unit relative to the bed.

14. The apparatus of claim 1, further comprising a reading light coupled to the handle.

15. The apparatus of claim 1, wherein the control unit includes an arm member, and said surface is a top surface of the arm member.

16. The apparatus of claim 1, wherein the at least one adjustment switch includes up and down adjustment switches are located on the surface of the control unit.

17. The apparatus of claim 1, further comprising a rotatable actuator coupled to the control unit, the adjustment switch being located within the rotatable actuator.

18. The apparatus of claim 1, further comprising a telephone coupled to the control unit.

19. The apparatus of claim 1, further comprising a card reader coupled to the control unit.

20. The apparatus of claim 1, further comprising a mounting tube coupled to the control unit, the mounting tube being configured to couple the control unit to a bar on the bed for a pivotable movement about a pivot axis.

5 21. The apparatus of claim 1, further comprising a headphone coupled to the control unit.

22. The apparatus of claim 1, further comprising an L-shaped connector pivotably coupled to the control unit and an arm coupled to the second leg of the L-shaped connector, the control unit extending over the arm.

10 23. The apparatus of claim 22, wherein the arm is a telescoping arm.

24. The apparatus of claim 1, further comprising touch screen control panel located on the surface.

15 25. A communication and control apparatus for use by a person located on a bed to control at least one function, the bed including a siderail, the apparatus comprising:

a control unit configured to control the at least one function; and

20 a linkage including an arm having a first end and a second end, a first coupler configured to the first end of the arm to the siderail about two pivot axes, a second coupler configured to couple the second end of the arm to the control unit about two pivot axes, the control unit being movable from a storage position adjacent to sidewall to a use position spaced apart from the sidewall by the linkage.

26. The apparatus of claim 25, wherein the control unit includes a curved top portion configured to receive a top rail of the siderail therein.

25 27. The apparatus of claim 25, wherein the control unit includes a recessed portion configured to receive the arm therein when the control unit is in its storage position.

28. The apparatus of claim 25, wherein the control unit includes a plurality of switches to control a plurality of functions, the switches being located on a surface of the control unit the is aligned at a transverse angle relative to a plane of the
30 siderail.

29. The apparatus of claim 25, wherein the linkage includes a channel pivotably coupled to the siderail about a first pivot axis, the first end of the arm being pivotably coupled to the channel about a second pivot axis, and a connector

pivotably coupled to the control unit about a third pivot axis, the second end of the arm being pivotably coupled to the connector about a fourth pivot axis so that the control unit is movable up and down and side to side relative to the siderail.

30. The apparatus of claim 25, wherein the linkage includes two
5 parallel arms connected between the siderail and the control unit.

31. The apparatus of claim 25, further comprising a speaker
coupled to the siderail.

32. The apparatus of claim 25, further comprising a light coupled to
the siderail.

10 33. The apparatus of claim 25, wherein the control unit has a
surface accessible to the person on the bed, the control unit further including a
plurality of icons located on the surface of the control unit, each icon representing a
separate one of a plurality of controlled functions, an indicator associated with each
icon, a single select switch located on the surface of the control unit, the select switch
15 being actuatable to scroll sequentially through the plurality of different functions, the
control unit being configured to actuate the indicator corresponding to a function
selected as the select switch is actuated to scroll through the plurality of different
controlled functions, and at least one adjustment switch located on the control unit to
control the function selected using the select switch.

20 34. The apparatus of claim 25, wherein the control unit controls a
plurality of functions including at least one of calling a nurse, turning on a light in a
room, turning on a reading light, controlling a TV, controlling a radio, placing and
receiving telephone calls, controlling drapes, controlling doors, adjusting a height of
the bed, adjusting a configuration of an articulating deck on the bed, adjusting a
25 mattress located on the bed, connecting to the Internet, and controlling a video game.

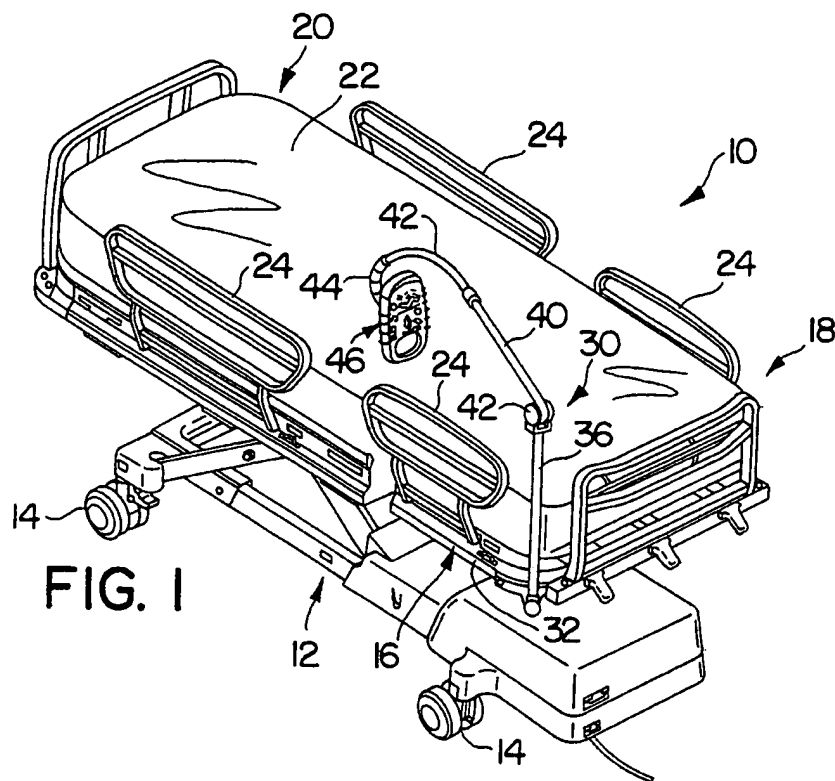


FIG. 1





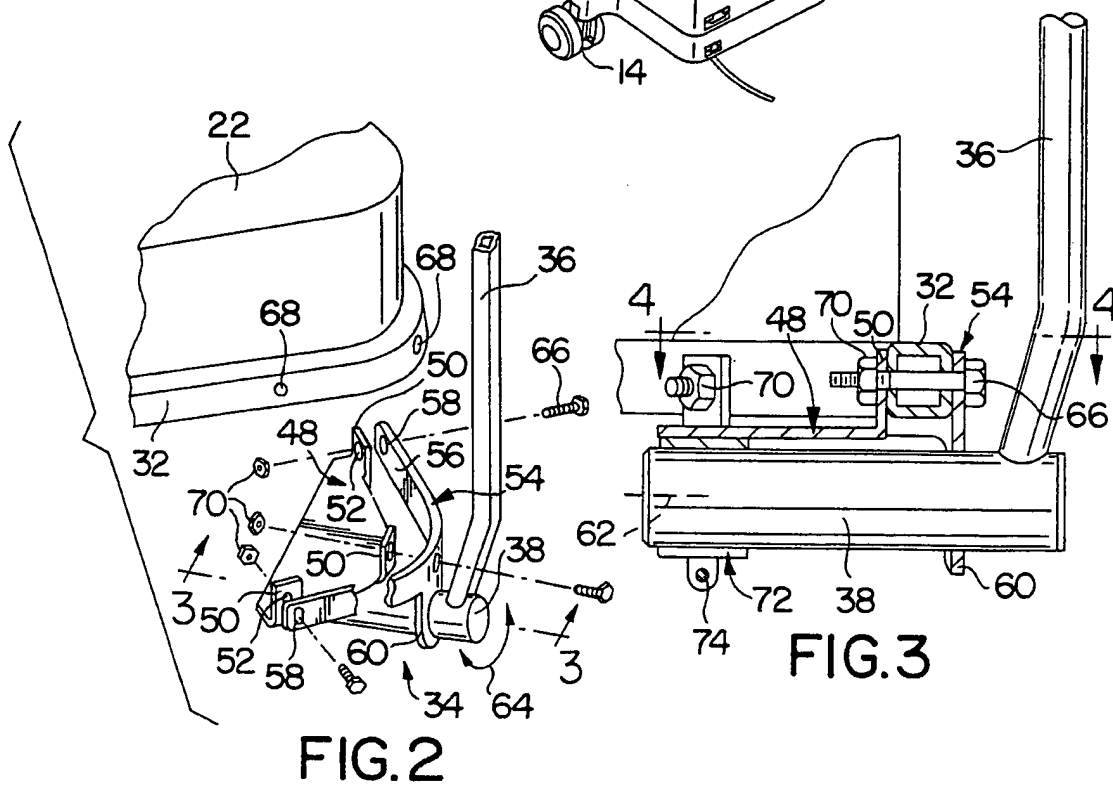




FIG. 2

FIG. 3

2/15

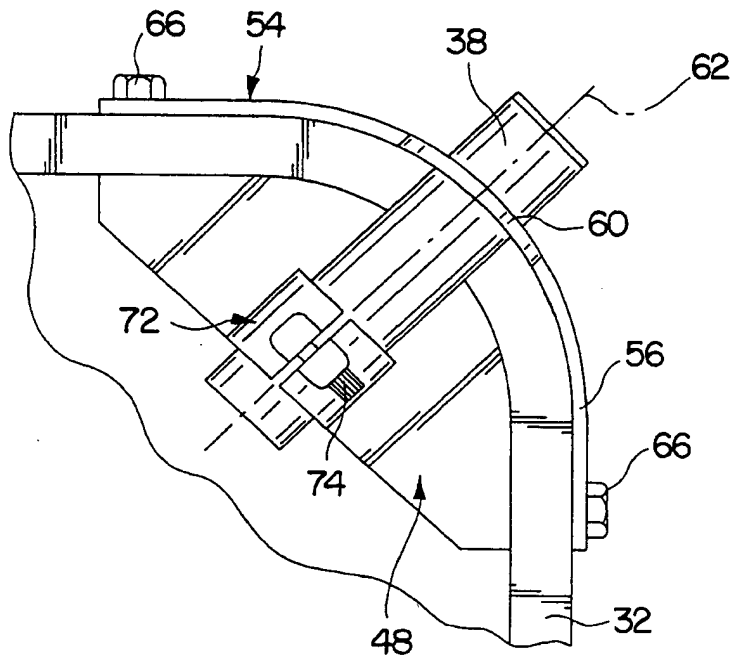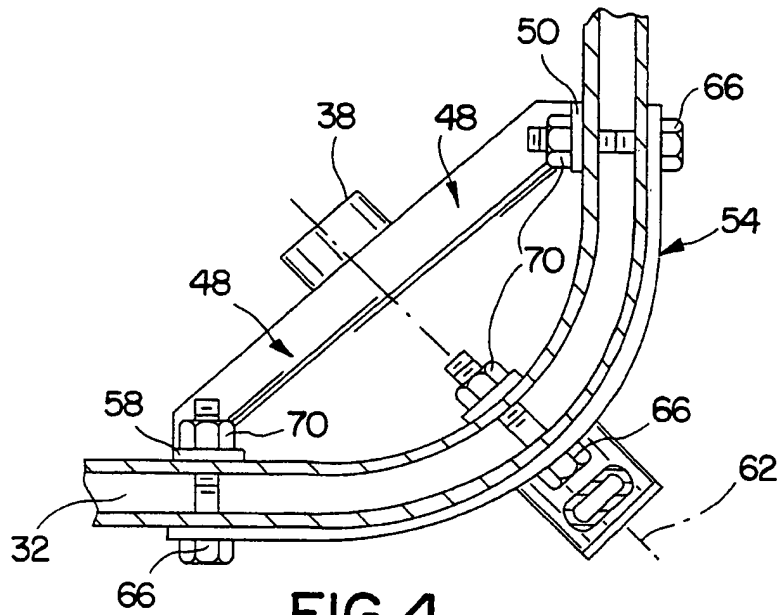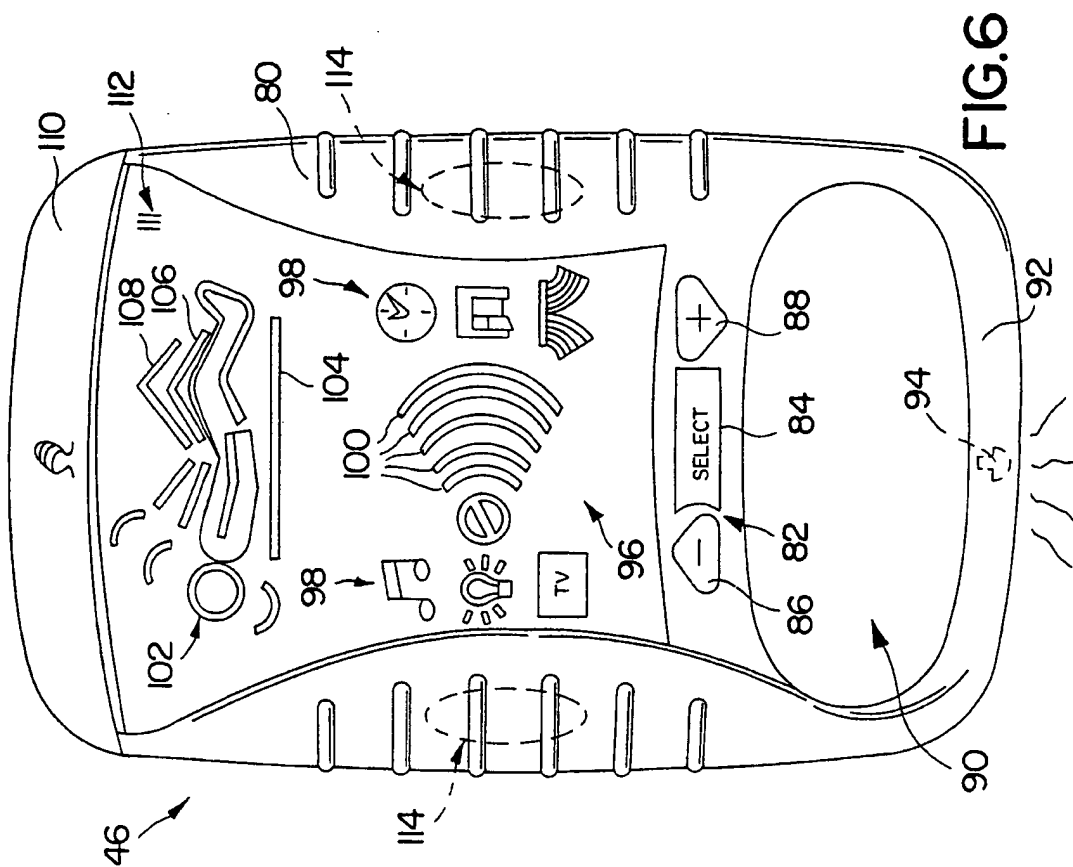

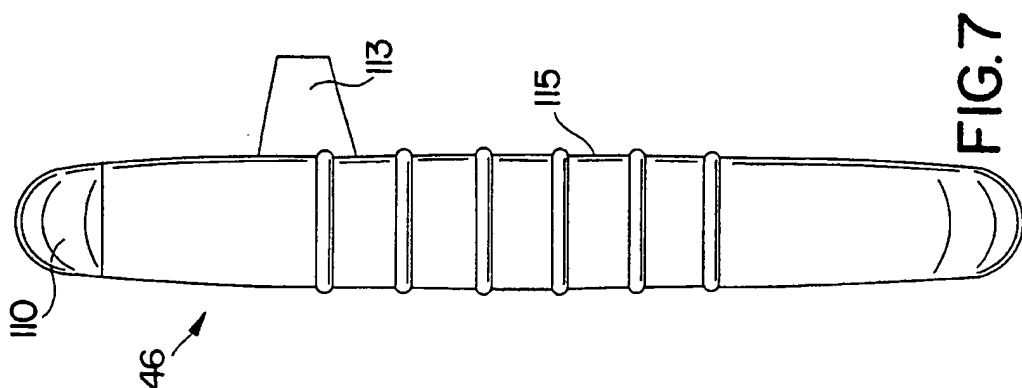

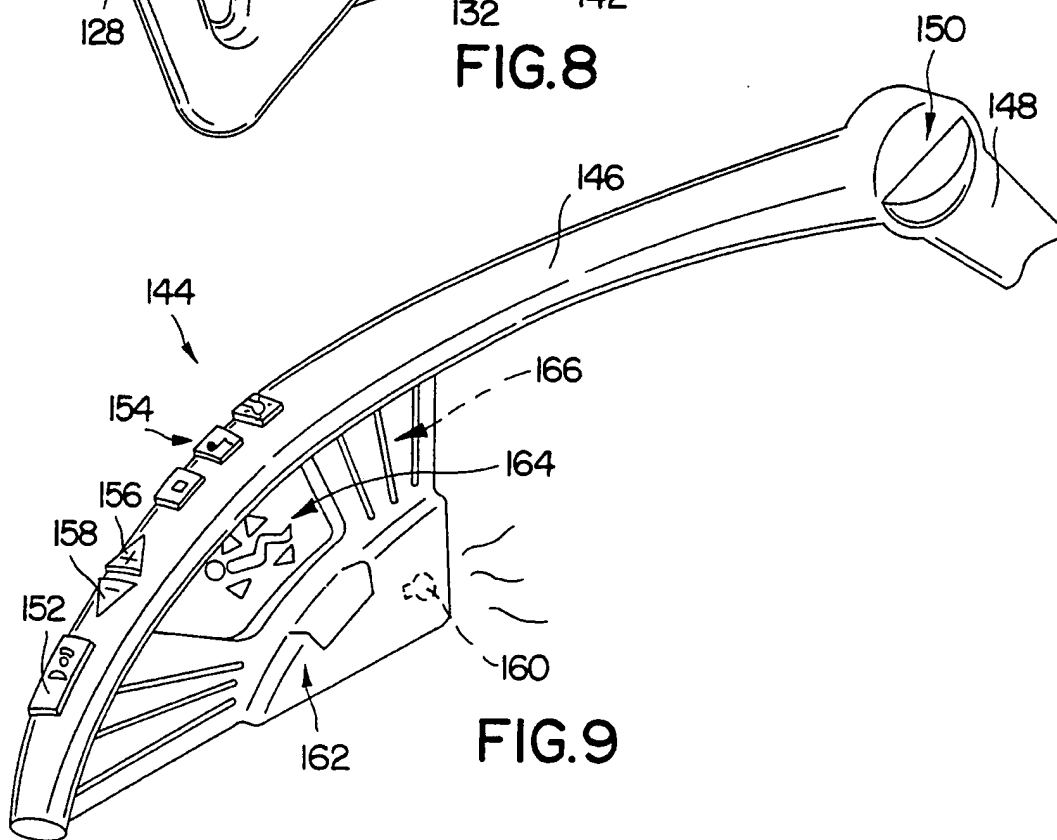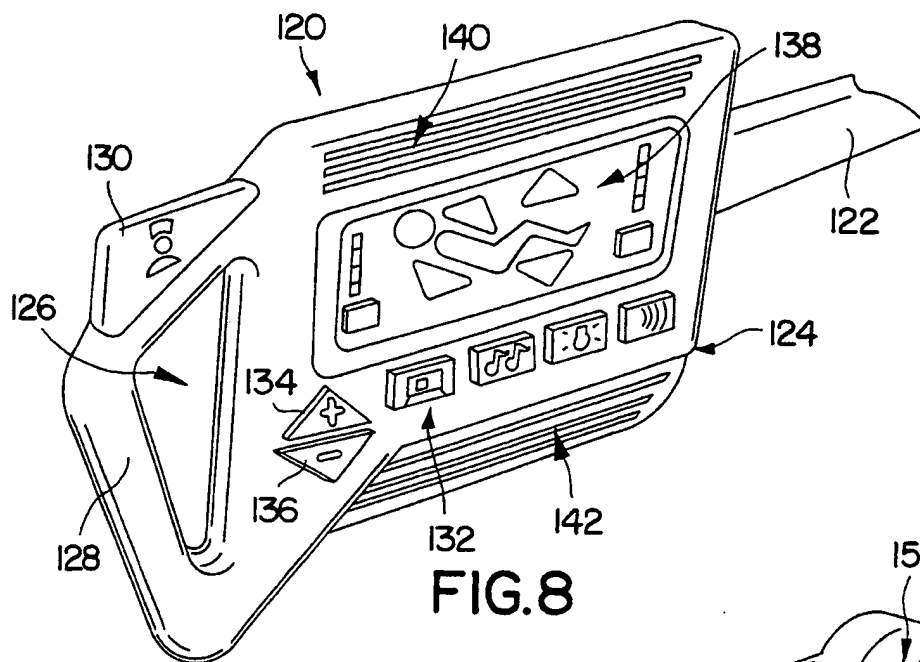

5/15

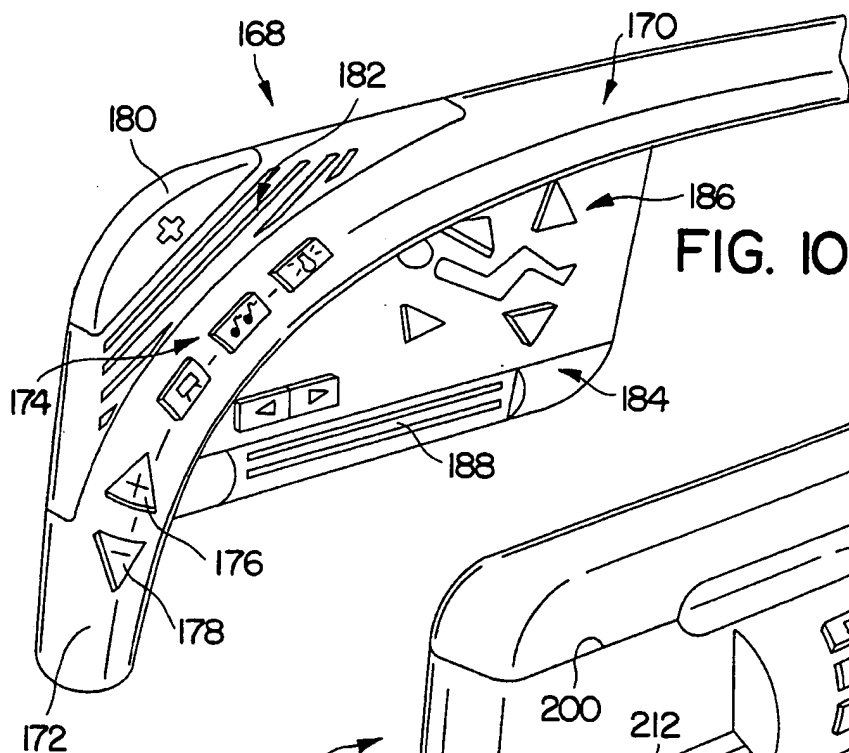


FIG. 10

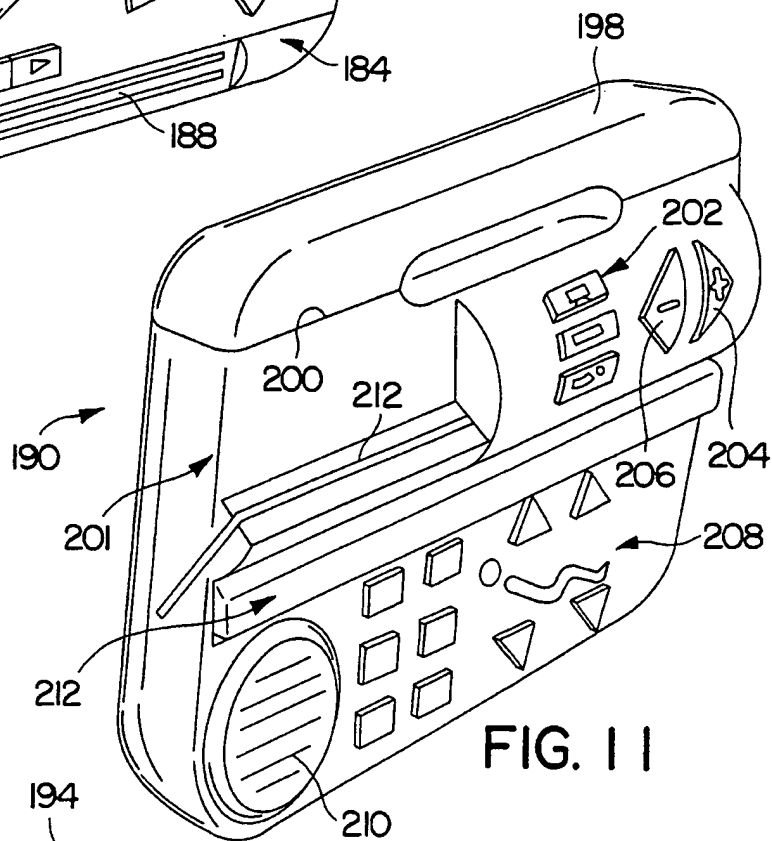


FIG. 11

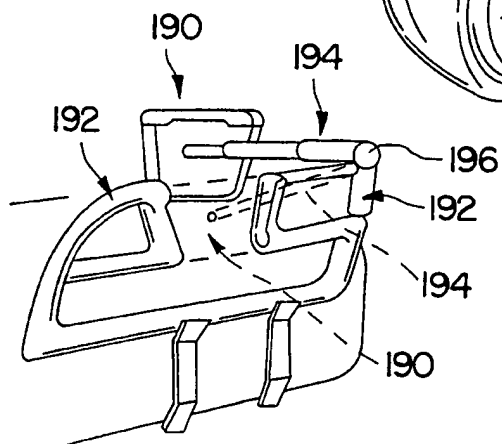


FIG. 12

6/15

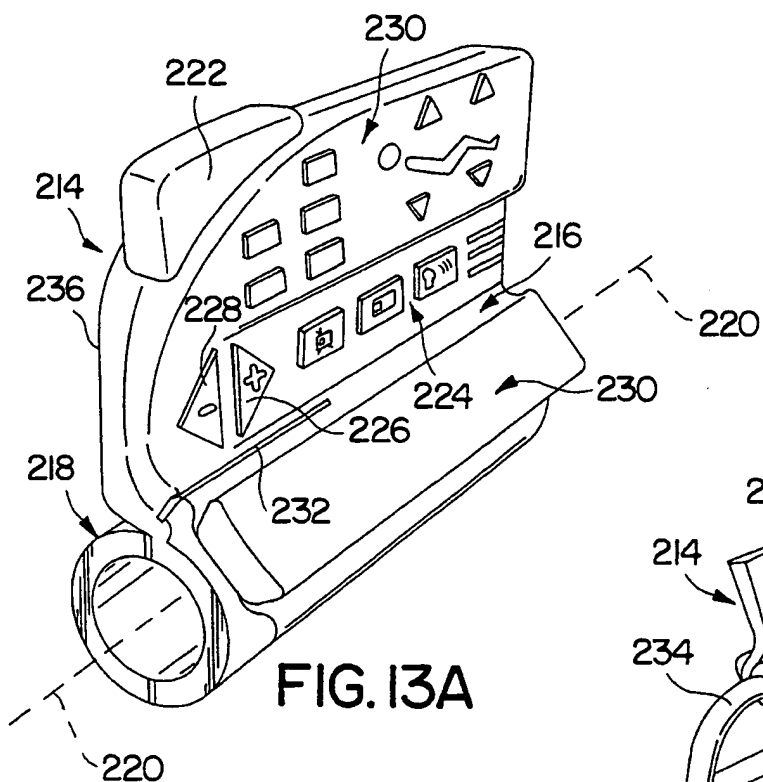


FIG. 13A

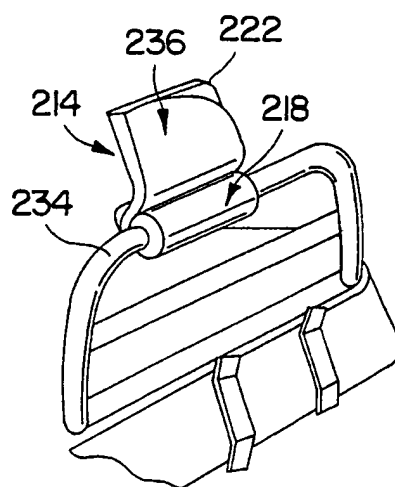


FIG. 13B

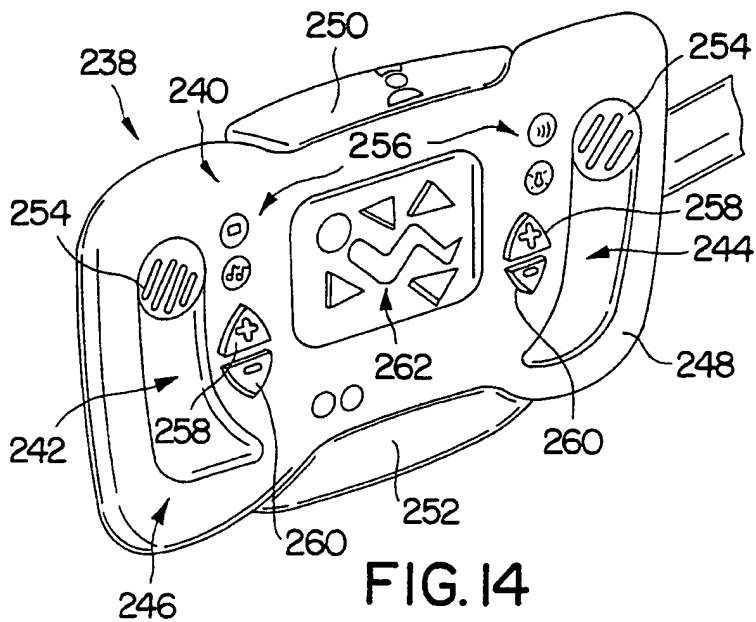


FIG. 14

7/15

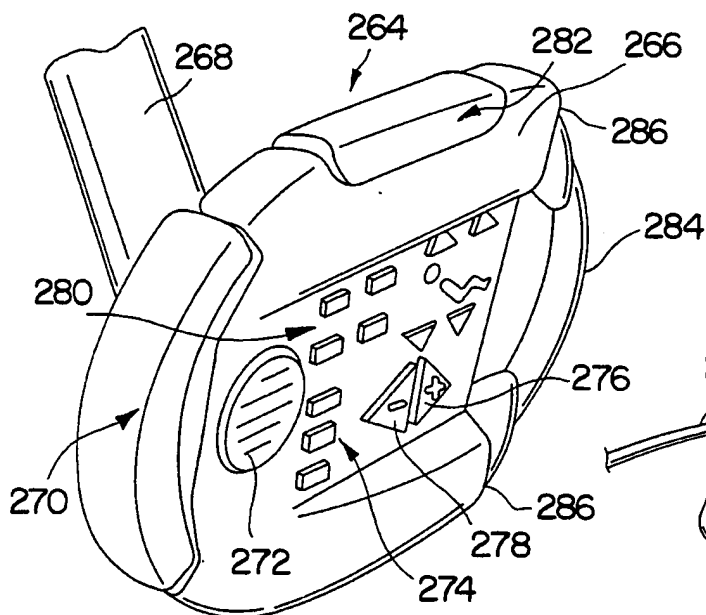


FIG. 15

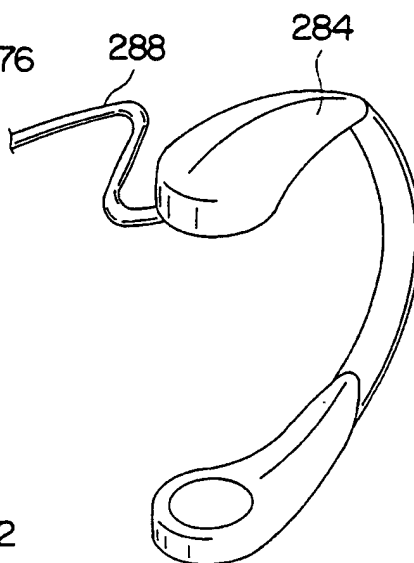


FIG. 16

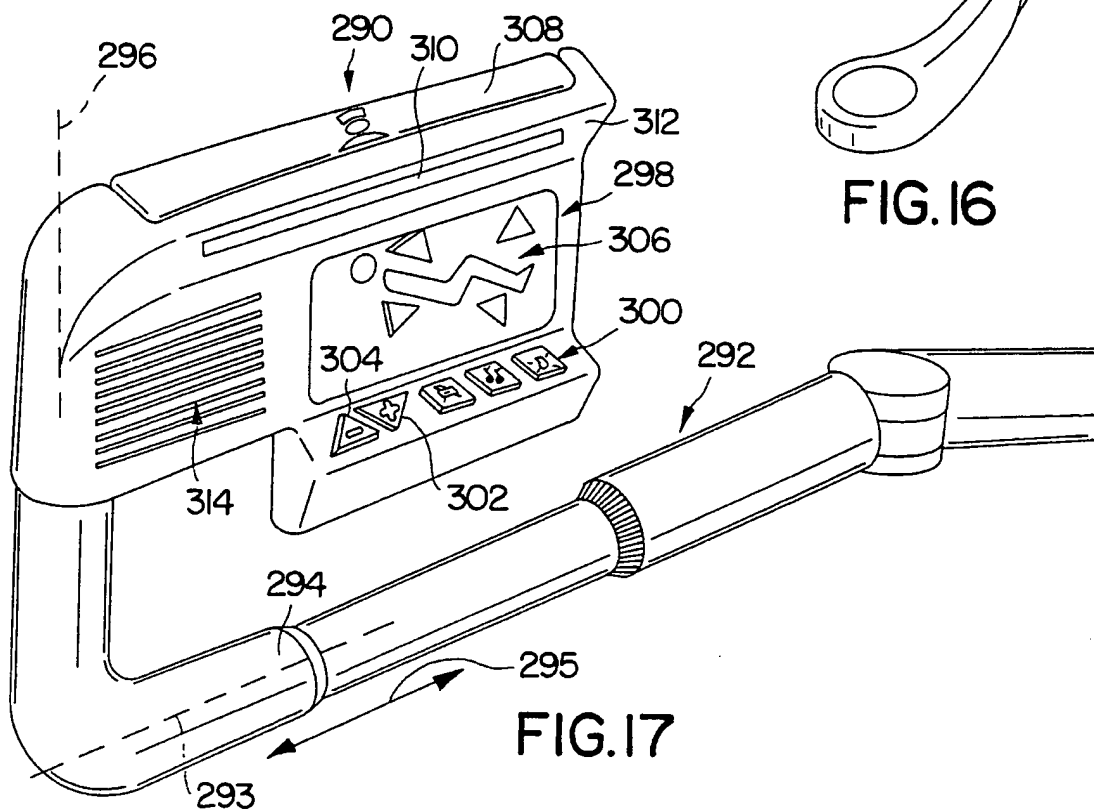
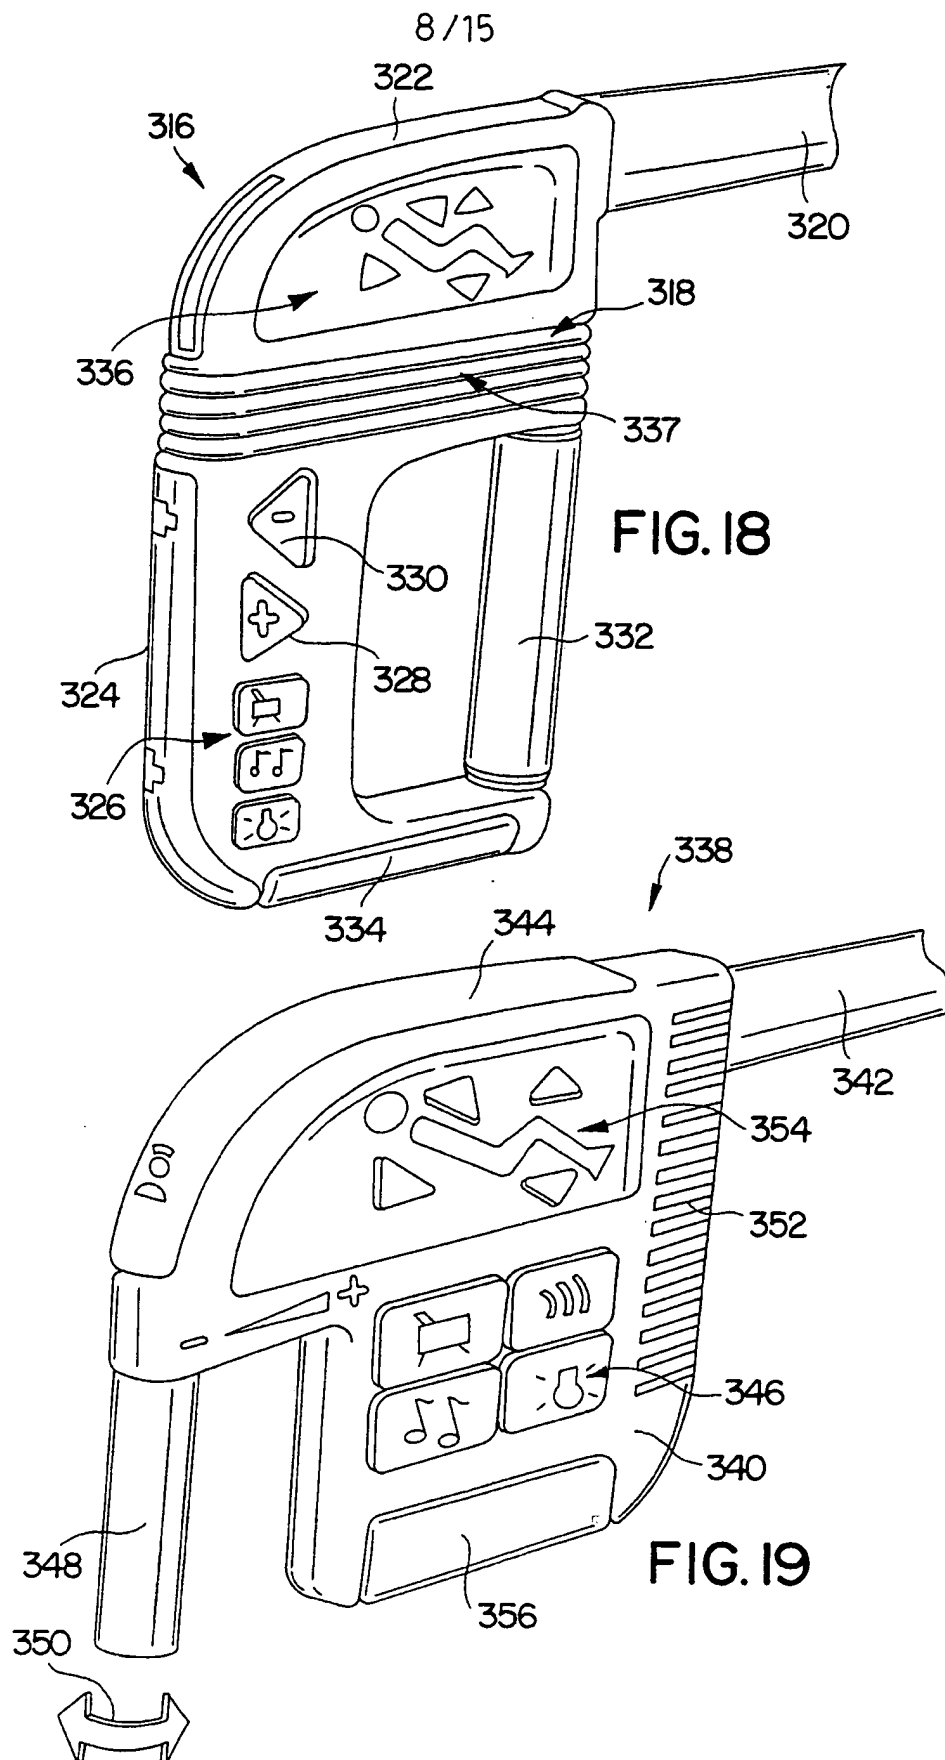
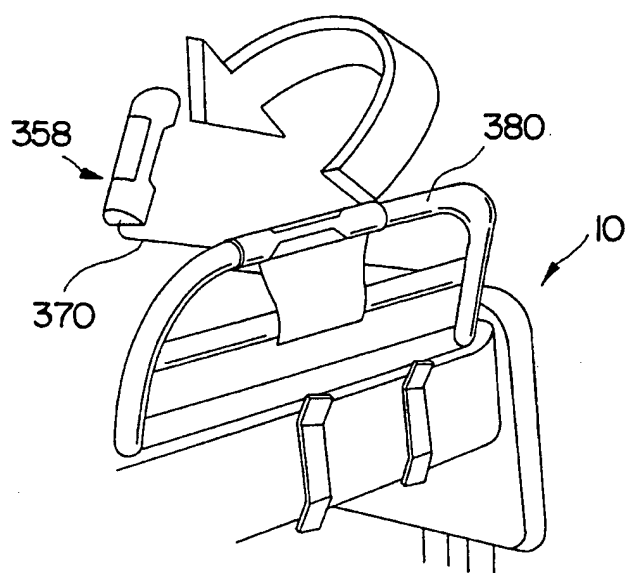
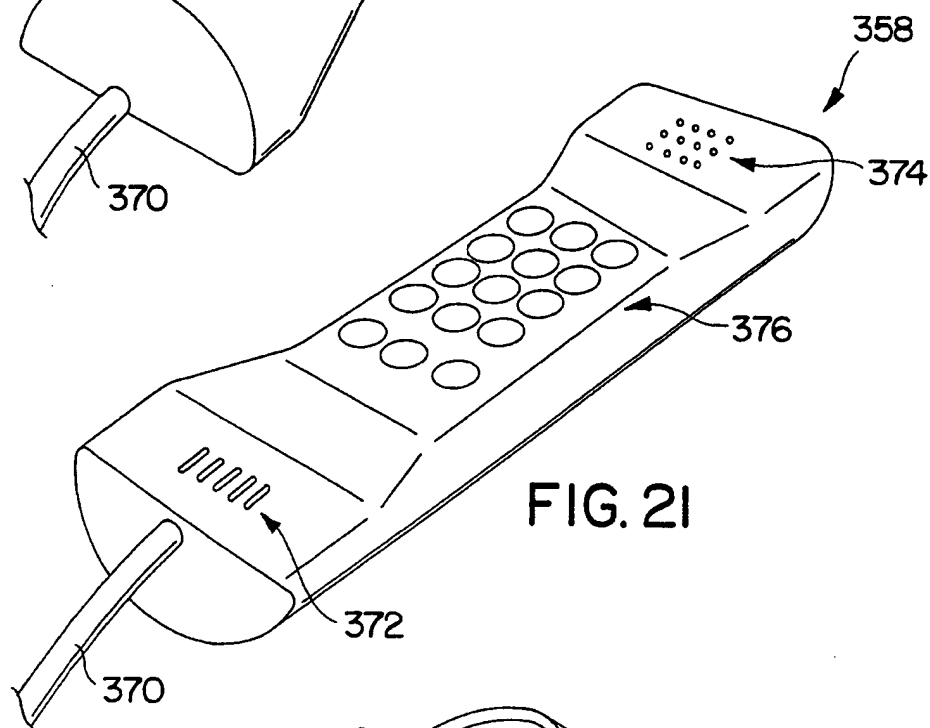
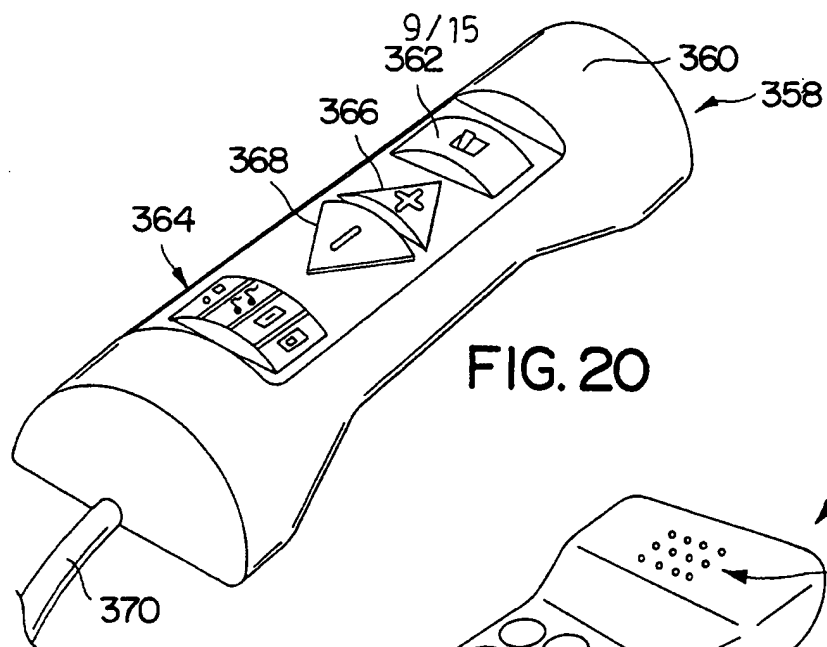


FIG. 17





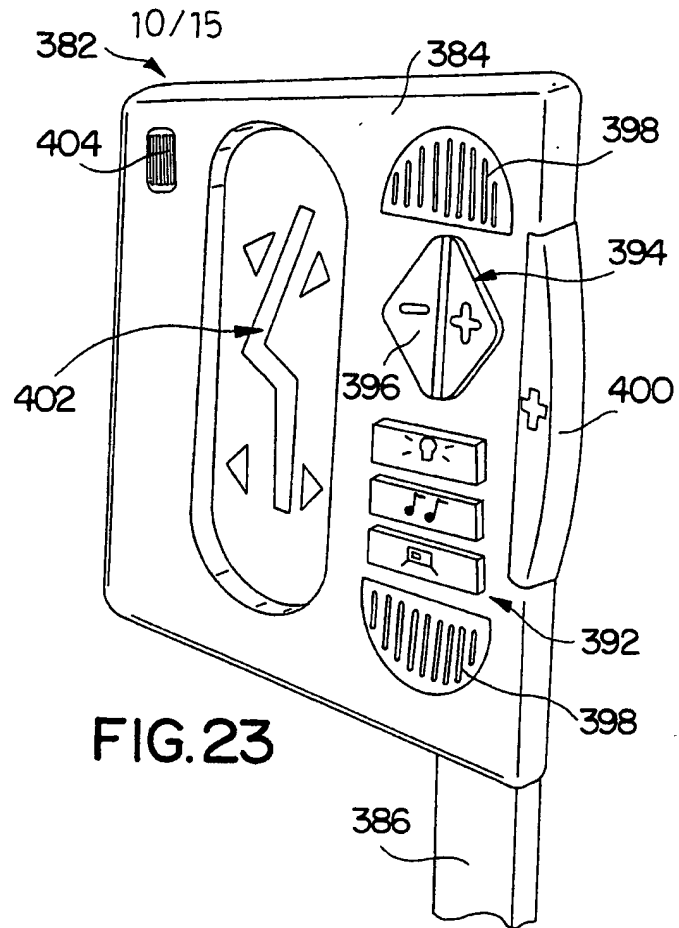


FIG. 23

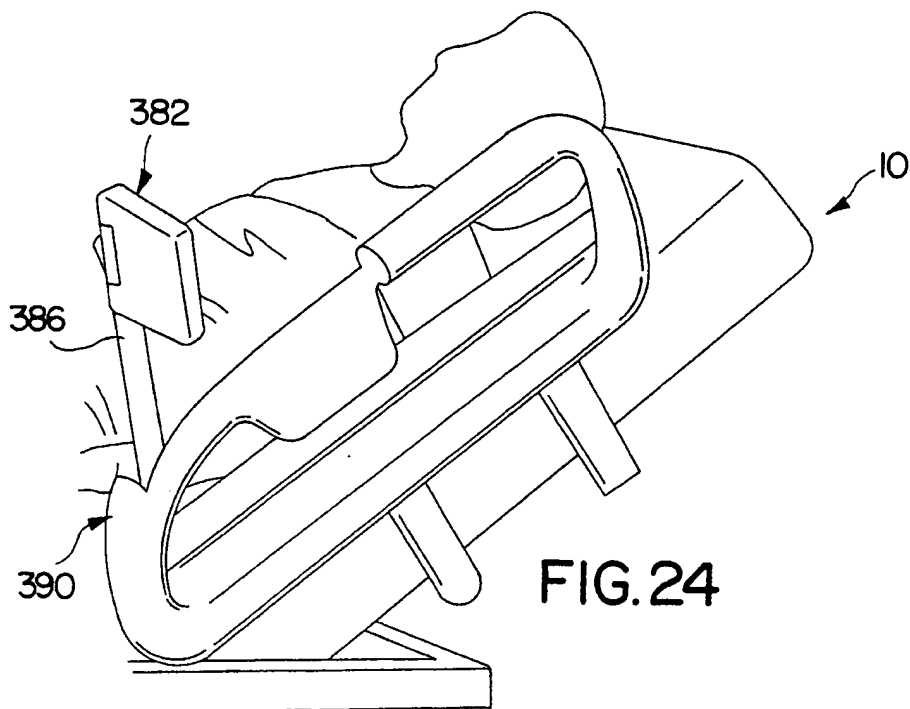


FIG. 24

11/15

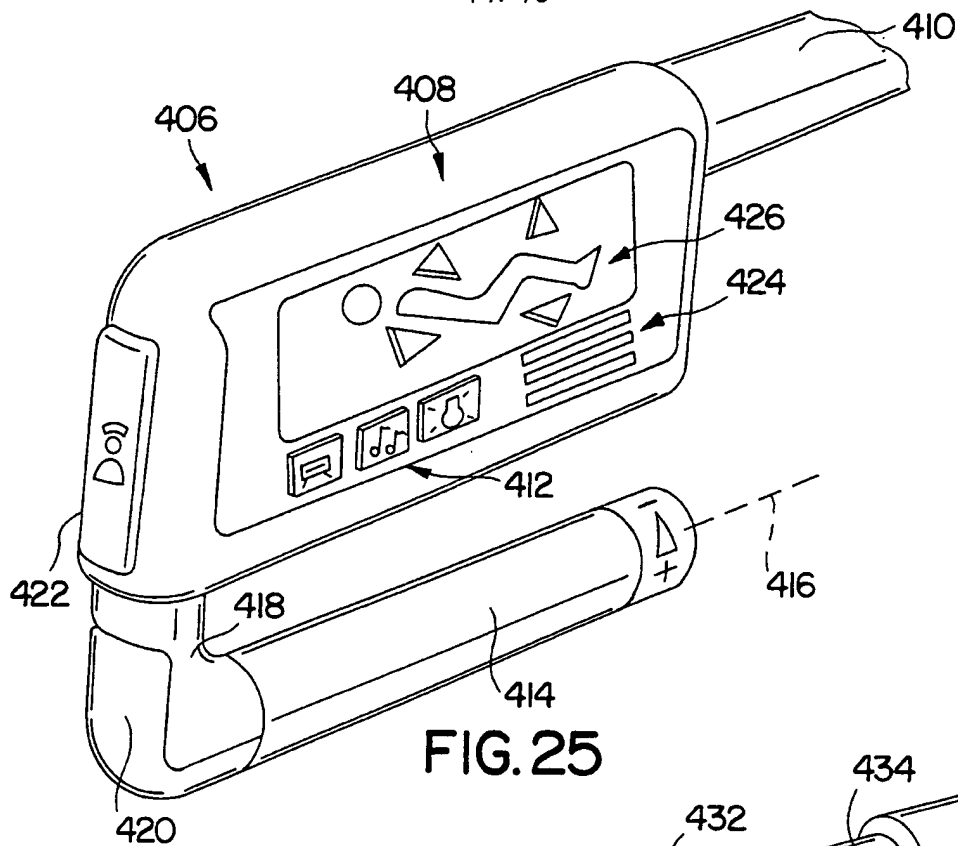


FIG. 25

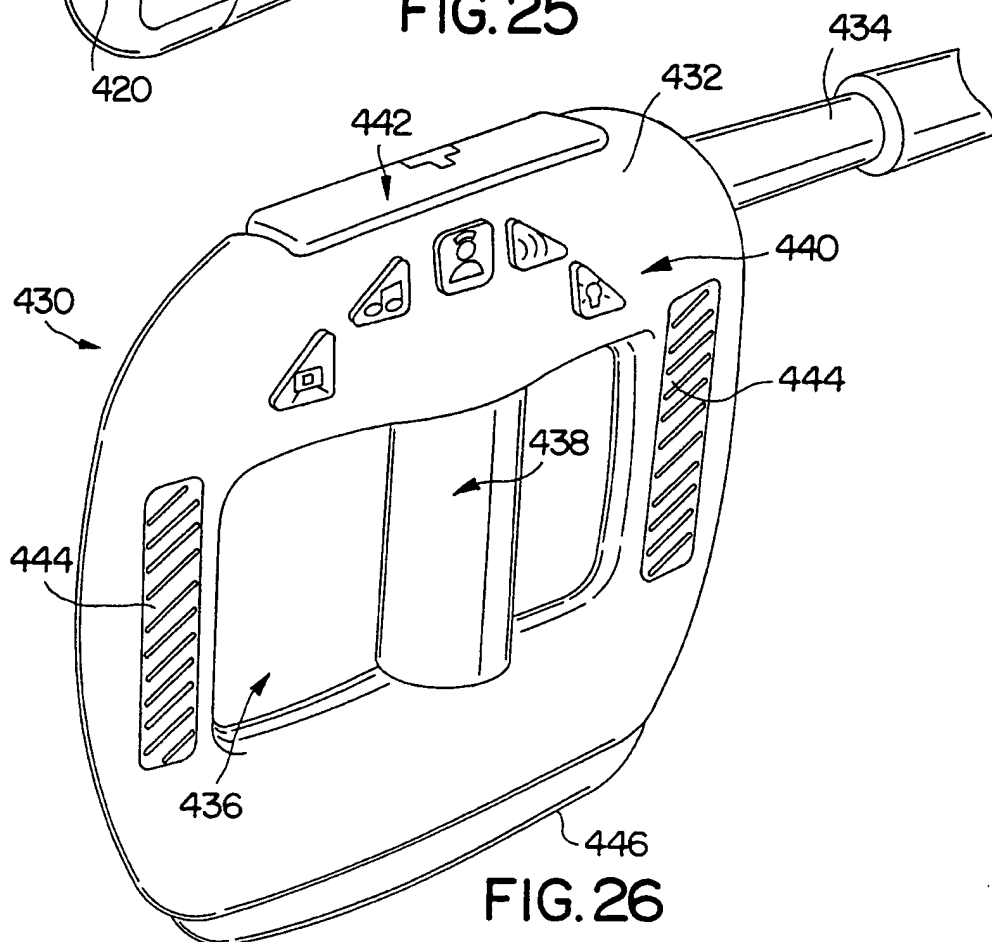


FIG. 26

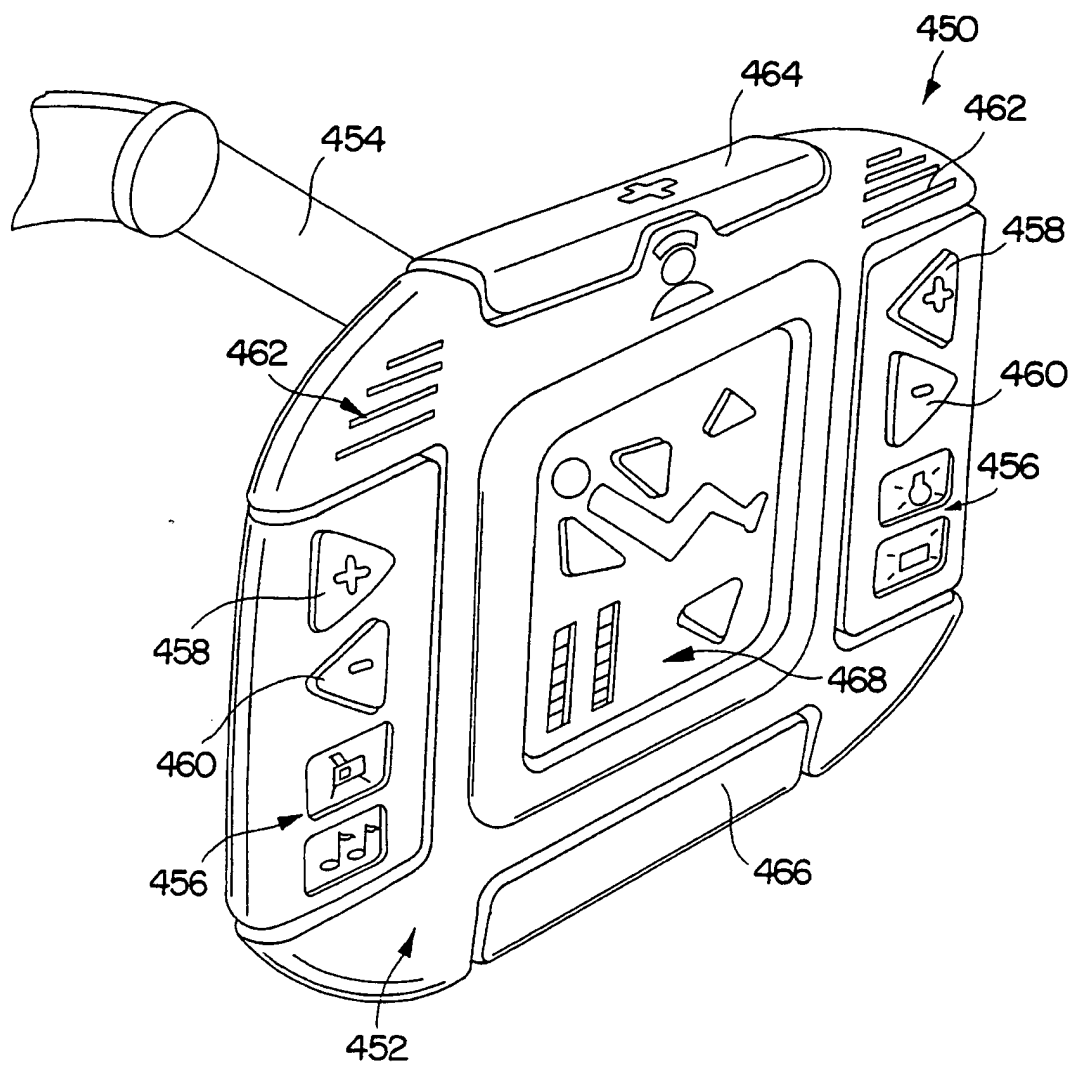


FIG. 27

13/15

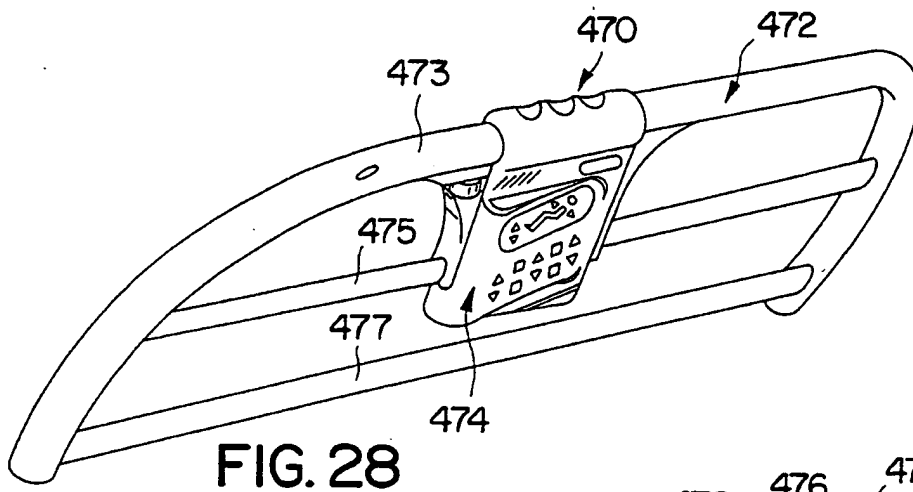


FIG. 28

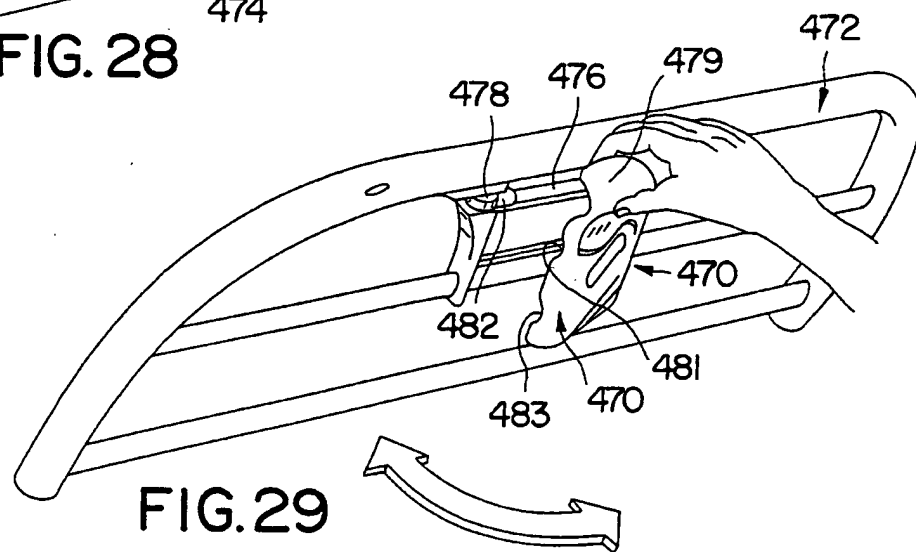


FIG. 29

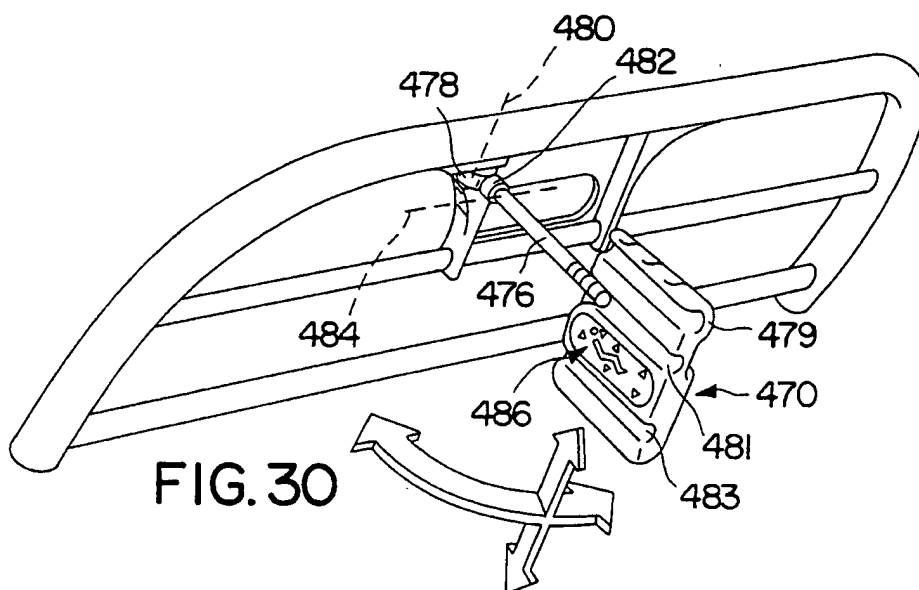


FIG. 30

14 / 15

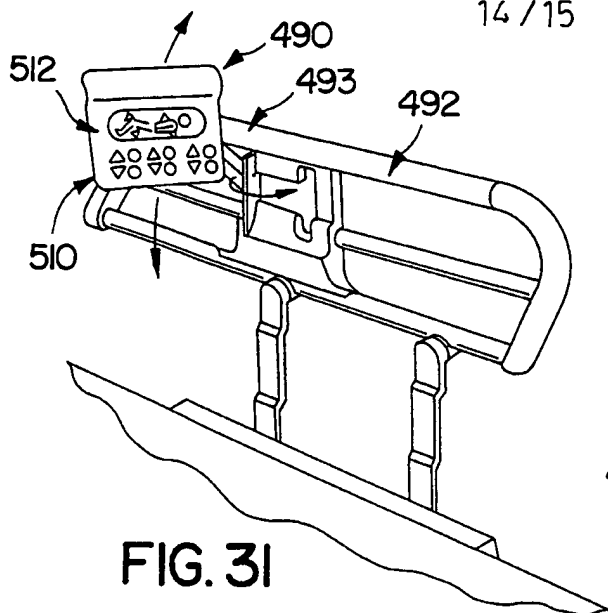


FIG. 31

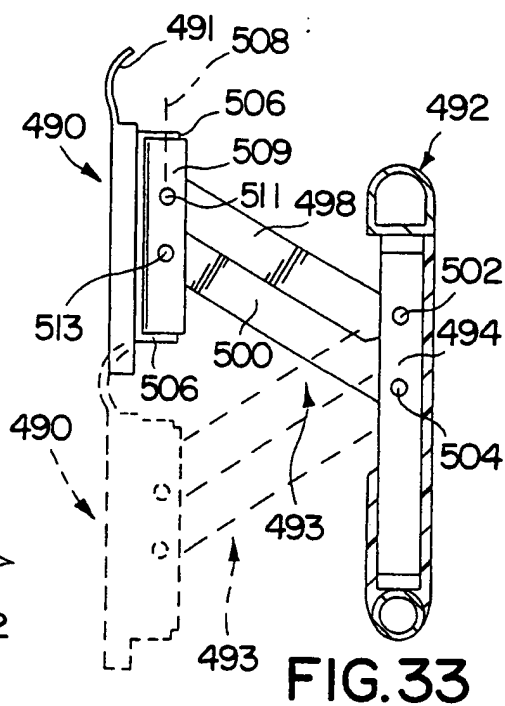


FIG. 33

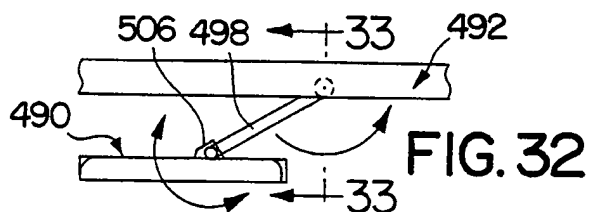


FIG. 32

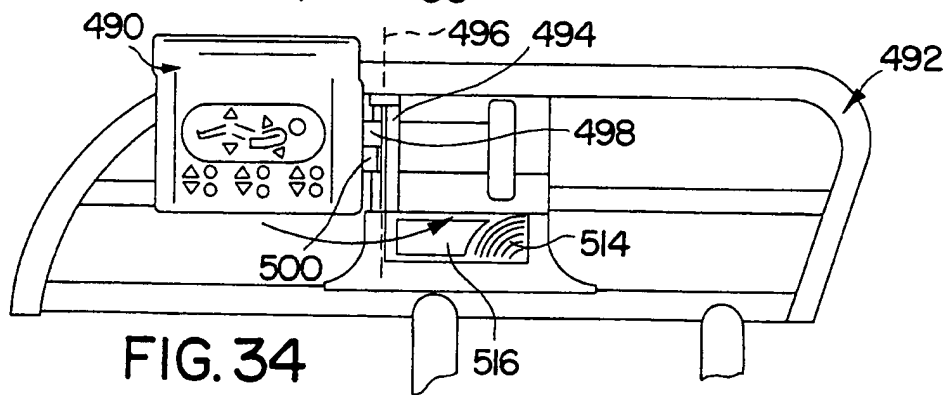


FIG. 34

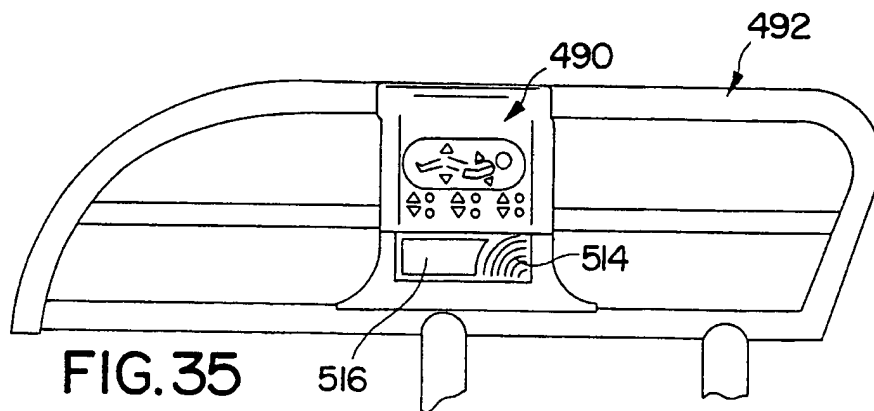


FIG. 35

15/15

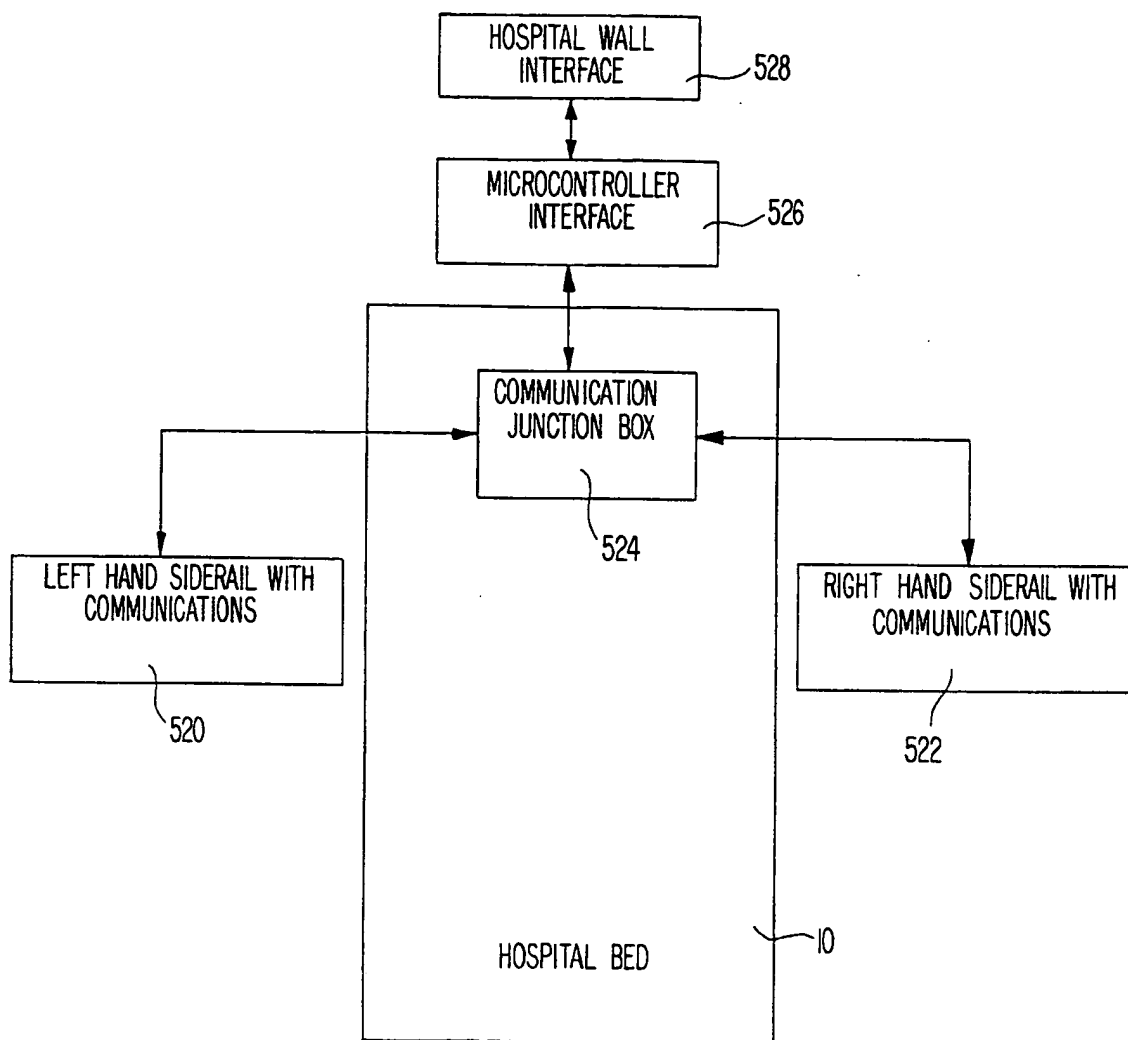


FIG. 36

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 99/08125

A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 A61G7/05

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 A61G H04M H01H

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4 183 015 A (DREW WILLIAM D ET AL) 8 January 1980 (1980-01-08) column 3, line 15 - line 61 column 5, line 25 - line 31; figures 2,3 ---	1,4,5,9, 25,31,34
A	EP 0 780 111 A (LE COUVIOUR SA) 25 June 1997 (1997-06-25) column 4, line 53 - column 6, line 41; figures ---	1-3
A	US 5 239 300 A (BERGER REIMAR ET AL) 24 August 1993 (1993-08-24) cited in the application the whole document --- -/--	1

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

18 August 1999

Date of mailing of the international search report

26/08/1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl.
Fax: (+31-70) 340-3016

Authorized officer

Baert, F

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US 99/08125

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 542 138 A (PARRISH GEORGE R ET AL) 6 August 1996 (1996-08-06) cited in the application the whole document ---	1
A	US 4 680 790 A (PACKARD RICHARD F ET AL) 14 July 1987 (1987-07-14) cited in the application the whole document ---	1
A	US 5 592 153 A (WELLING JEFFREY R ET AL) 7 January 1997 (1997-01-07) cited in the application the whole document -----	1

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 99/08125

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 4183015 A	08-01-1980	JP 55005689 A	16-01-1980
EP 0780111 A	25-06-1997	AT 172868 T	15-11-1998
		DE 59504163 D	10-12-1998
		ES 2123893 T	16-01-1999
US 5239300 A	24-08-1993	AT 127007 T	15-09-1995
		DE 3941117 A	21-06-1990
		WO 9006739 A	28-06-1990
		DE 8915340 U	28-06-1990
		DE 58909412 D	05-10-1995
		EP 0376066 A	04-07-1990
		ES 2079371 T	16-01-1996
		GR 3018266 T	29-02-1996
		JP 3502844 T	27-06-1991
US 5542138 A	06-08-1996	NONE	
US 4680790 A	14-07-1987	NONE	
US 5592153 A	07-01-1997	NONE	